


AUTOSAMPLER PRECISION

10 INJECTIONS

Max = 0.12%

Min = -0.10%

%RSD= 0.07%

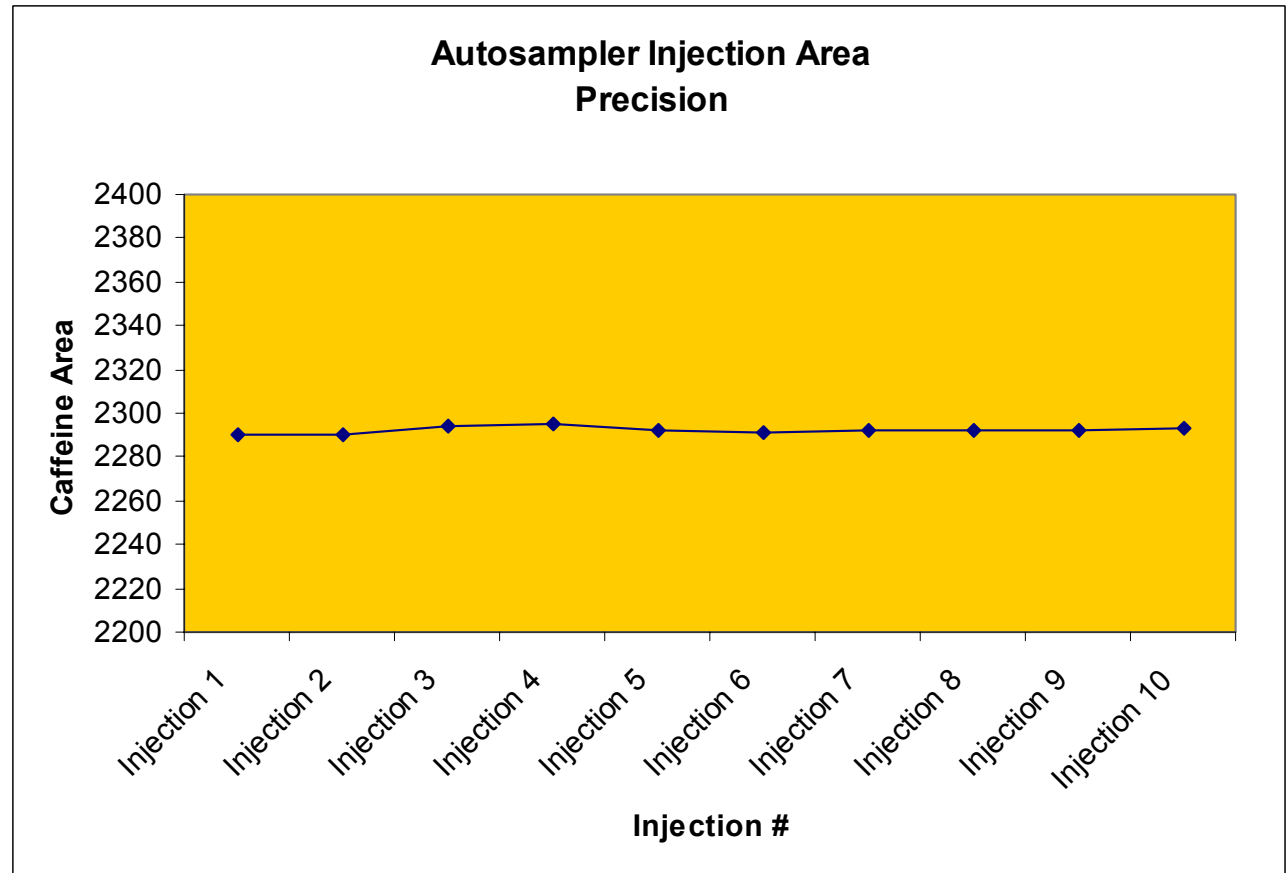

103 Brighton Avenue
Long Branch, NJ 07740 USA
732-229-3400 Fax. 732-229-2403
Email: info@microsolvtch.com
www.microsolvtch.com